

350-ADA-1

*Dual-ramp ADA Compliant Wheelchair Scale
Software Version 11525*

Technical Manual



© Rice Lake Weighing Systems. All rights reserved.

Rice Lake Weighing Systems® is a registered trademark of
Rice Lake Weighing Systems.

All other brand or product names within this publication are trademarks or
registered trademarks of their respective companies.

All information contained within this publication is, to the best of our knowledge, complete and
accurate at the time of publication. Rice Lake Weighing Systems reserves the right to make
changes to the technology, features, specifications and design of the equipment without notice.

Revision History

This section tracks and describes the current and previous manual revisions for awareness of major updates and when the updates took place.

| Revision | Date | Description |
|----------|-------------------|---|
| A | December 4, 2025 | Initial manual release with product; software version 11525 |
| B | February 10, 2026 | Updated platform dimensions |
| | | |
| | | |

Table i. Revision Letter History

Contents

| | | |
|------------|--|-----------|
| 1.0 | Introduction | 5 |
| 1.1 | Safety | 5 |
| 1.2 | FCC Compliance | 6 |
| 1.3 | Disposal | 6 |
| 2.0 | Assembly | 7 |
| 2.1 | Unpacking | 7 |
| 2.1.1 | Repacking | 11 |
| 2.2 | Scale Setup | 11 |
| 2.2.1 | Attaching Feet to the Scale | 11 |
| 2.2.2 | Installing Ramps onto the Scale | 12 |
| 2.2.3 | Leveling the Scale Base | 12 |
| 2.2.4 | Hinge Setup | 13 |
| 2.2.5 | Insert Alkaline Batteries | 14 |
| 2.2.6 | Power Connection | 14 |
| 3.0 | Operation | 15 |
| 3.1 | Key Descriptions | 15 |
| 3.2 | Weighing | 16 |
| 3.3 | Hold/Release Function | 16 |
| 3.4 | Preset Tare | 16 |
| 3.5 | Toggle Tare | 16 |
| 3.6 | Using the Body Mass Index (BMI) Function | 17 |
| 3.6.1 | LB Mode | 17 |
| 3.6.2 | KG Mode | 17 |
| 3.7 | Troubleshooting | 18 |
| 4.0 | Configuration | 19 |
| 4.1 | Setup Switch | 19 |
| 4.2 | General Navigation | 19 |
| 4.2.1 | Change Parameters | 19 |
| 4.2.2 | Enter Numbers | 19 |
| 4.2.3 | Save and Return to Main Menu | 19 |
| 4.3 | Configuration Mode | 20 |
| 4.4 | Programming Mode Menu | 21 |
| 4.5 | Default Menu | 24 |
| 4.6 | Scale Calibration | 24 |
| 4.7 | Test Menu | 25 |
| 5.0 | Communication | 26 |
| 5.1 | Push-button Keypad Print | 26 |
| 5.2 | Communication Protocols | 27 |
| 5.2.1 | Escape Protocol | 27 |
| 5.2.2 | Maintenance Protocol | 28 |
| 5.3 | USB Connection | 29 |
| 6.0 | Maintenance | 30 |
| 6.1 | Basic Maintenance | 30 |
| 6.2 | Cleaning | 30 |
| 6.3 | Periodic Maintenance | 30 |
| 7.0 | Specifications | 31 |

1.0 Introduction

The 350-ADA-1 digital wheelchair scale is a user-friendly, quality scale, designed for safe weighing of ambulatory and non-ambulatory patients. Movement compensation technology ensures sound, accurate weighments.

The scale is set up to use motion sensing technology, to determine actual weight of a moving patient. The weight can be displayed in pounds or kilograms. To obtain a tare weight, See [Section 3.0 on page 15](#).

The wheelchair scale has a unique folding feature that enables easy transportation and simplifies assembly, avoiding the need for field wiring and recalibration.



Manuals are available from Rice Lake Weighing Systems at www.ricelake.com/manuals

Warranty information is available at www.ricelake.com/warranties

1.1 Safety

Safety Definitions:



DANGER: Indicates an imminently hazardous situation that, if not avoided, will result in death or serious injury. Includes hazards that are exposed when guards are removed.



WARNING: Indicates a potentially hazardous situation that, if not avoided, could result in serious injury or death. Includes hazards that are exposed when guards are removed.



CAUTION: Indicates a potentially hazardous situation that, if not avoided, could result in minor or moderate injury.



IMPORTANT: Indicates information about procedures that, if not observed, could result in damage to equipment or corruption to and loss of data.

General Safety



Do not operate or work on this equipment unless this manual has been read and all instructions are understood. Failure to follow the instructions or heed the warnings could result in injury or death. Contact any Rice Lake Weighing Systems dealer for replacement manuals.



WARNING

Failure to heed could result in serious injury or death.

Ensure every individual who operates or works with this unit has read and understands all safety information.

Do not transport the scale while someone is on the scale.

Do not allow minors (children) or inexperienced persons to operate this scale.

Do not use in the presence of flammable materials.

Do not use this product if any of the components are loose or cracked.

Do not use near water.

Do not use the scale on slippery surfaces, such as a wet floor.

Do not use this scale when a person's body or feet are wet, such as after taking a bath.

Do not place fingers into slots or possible pinch points.

To avoid cross contamination, the scale should be cleaned regularly.

Prior to cleaning, make sure the scale is disconnected from the power source.

People with disabilities, or who are physically fragile, should always be assisted by another person when using this scale.

**IMPORTANT**

Do not drop the scale or subject it to violent shocks.

Do not jump on the scale.

For accurate weighing, the scale must be placed on a flat, stable surface.

Operating at voltages and frequencies other than specified could damage the equipment.

Avoid contact with excessive moisture.

Do not make alterations or modifications to the scale.

Rice Lake Weighing Systems offers optional AC adapters; utilizing an adapter not supplied by Rice Lake Weighing Systems voids all warranties and approvals.

Weight exceeding the maximum capacity may damage the scale.

1.2 FCC Compliance

United States

This equipment has been tested and found to comply with the limits for a Class A digital device, pursuant to Part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference when the equipment is operated in a commercial environment. This equipment generates, uses, and can radiate radio frequency energy and, if not installed and used in accordance with the instruction manual, may cause harmful interference to radio communications. Operation of this equipment in a residential area is likely to cause harmful interference in which case the user will be required to correct the interference at his own expense.

Canada

This digital apparatus does not exceed the Class A limits for radio noise emissions from digital apparatus set out in the Radio Interference Regulations of the Canadian Department of Communications.

Le présent appareil numérique n'émet pas de bruits radioélectriques dépassant les limites applicables aux appareils numériques de la Class A prescrites dans le Règlement sur le brouillage radioélectrique édicté par le ministère des Communications du Canada.

1.3 Disposal



Product Disposal

The product must be brought to appropriate separate waste collection centers at the end of its life cycle.

Proper separate collection to recycle the product helps prevent possible negative effects on the environment and to health, and promotes the recycling of the materials. Users who dispose of the product illegally shall face administrative sanctions as provided by law.

Battery Disposal

Dispose of batteries at appropriate waste collection centers at the end of their life cycle in accordance with local laws and regulations. Batteries and rechargeable batteries may contain harmful substances that should not be disposed of in household waste. Batteries may contain harmful substances including but not limited to: cadmium (Cd), lithium (Li), mercury (Hg) or lead (Pb). Users who dispose of batteries illegally shall face administrative sanctions as provided by law.



WARNING: Risk of fire and explosion. Do not burn, crush, disassemble or short-circuit lithium batteries.

2.0 Assembly

Use the following information to unpack and set up the 350-ADA-1 digital wheelchair scale.

2.1 Unpacking

The following procedure describes how to unpack the scale and scale components from the shipping crate.

1. Place the unopened crate in an open area that has ample room for unpacking the scale.



NOTE: Due to its size, at least two people are recommended for unpacking the scale.

2. Use a Phillips drill bit to remove the ten screws securing the shipping crate cover (see [Figure 2-1](#)).

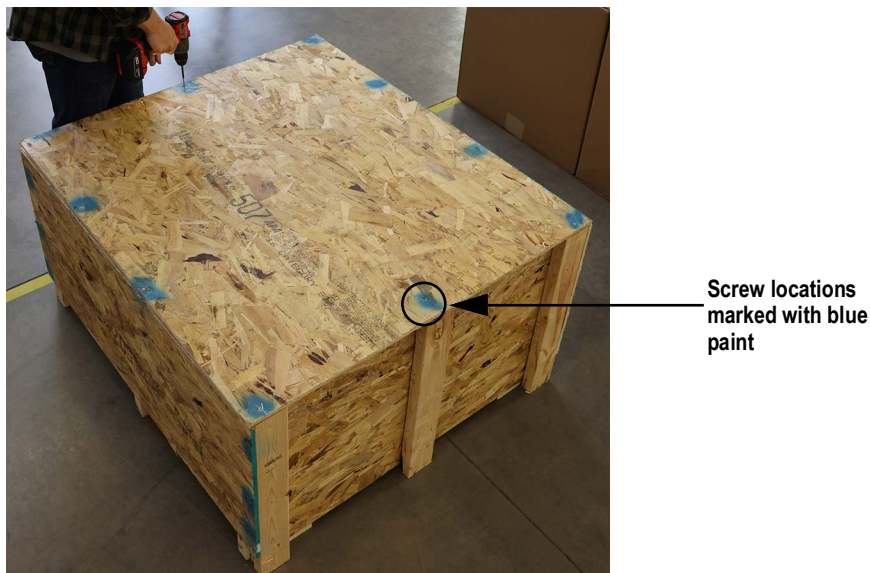


Figure 2-1. Crate Cover Screw Removal

3. Remove and set aside the crate cover.
4. Remove the two cardboard blocks.

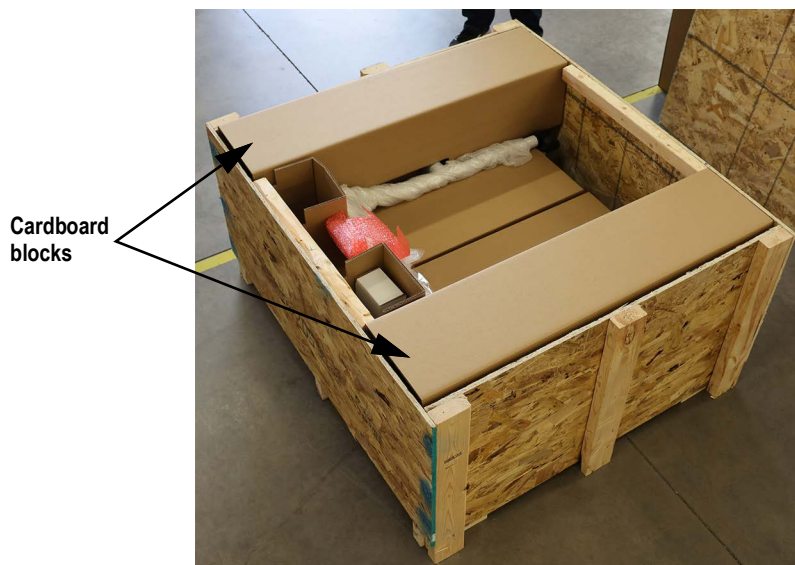


Figure 2-2. Opened Shipping Crate

5. Remove the six screws securing the side panel to the crate.



Figure 2-3. Side Panel Screw Removal

6. Remove and set aside the side panel.
7. Repeat [Step 5](#) and [Step 6](#) for the second side panel.
8. Locate and set aside the parts box and manual.

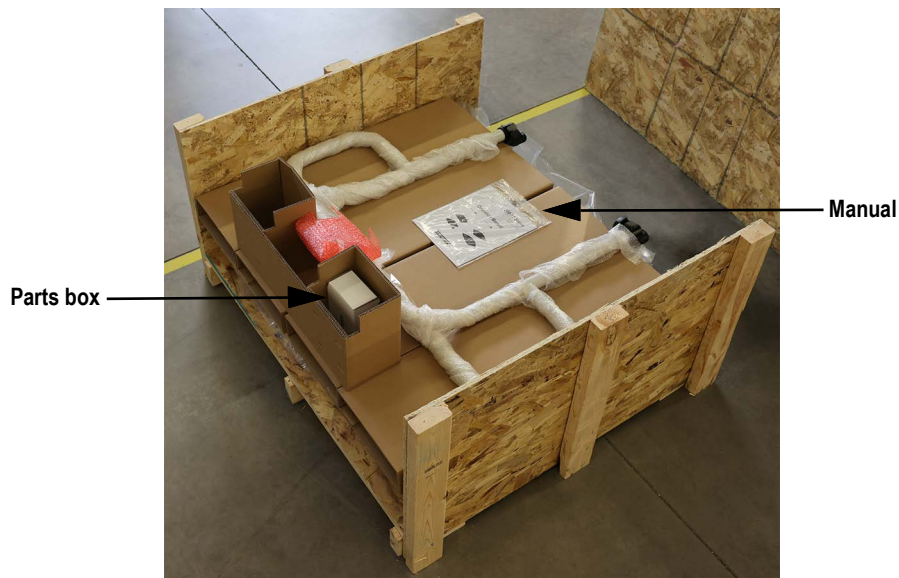


Figure 2-4. Crate with Side Panels Removed

9. Loosen the clamps to raise the handrail (see [Figure 2-5](#)).
10. Remove the four cardboard platforms.



Figure 2-5. Raising Handrail and Removing Cardboard Platforms

11. Lift and remove the scale ramps from the crate.



Figure 2-6. Unpacking Scale Ramp

12. Remove the remaining cardboard pieces.



NOTE: For ease of removal, fold the handrail back down before moving the scale.

13. With assistance, lift and remove the scale base from the crate and gently set it down on the floor (see [Figure 2-7](#)).



CAUTION: Rice Lake Weighing Systems recommends using two people for lifting the scale and to use proper lifting techniques to prevent injury.



IMPORTANT: Do not lift the scale out of the crate by its handrail as this can cause the hinges to break or affect the scale operation.



Figure 2-7. Unpacking Scale



NOTE: Visually inspect the scale to ensure all parts are included and undamaged. If parts were damaged in shipment, notify Rice Lake Weighing Systems and the shipper immediately.

Parts contained in the shipping crate include:

- * Scale
- * Manual
- * AA batteries (6) (see “Parts Inside” box in [Figure 2-8 on page 10](#))
- * Scale feet (4) (see “Parts Inside” box in [Figure 2-8 on page 10](#))
- * Scale ramps (2)
- * 5 mm Allen wrench (see “Parts Inside” box in [Figure 2-8 on page 10](#))
- * Allen bolt (10) (see “Parts Inside” box in [Figure 2-8 on page 10](#))



Figure 2-8. Parts Box

2.1.1 Repacking

Retain the packaging for use in the event that the scale must be returned or moved. The product must be properly packed with sufficient packing materials. Whenever possible, use the original carton and packing materials when shipping the scale back.

 **IMPORTANT:** *Damage caused by improper packaging is not covered by the warranty.*

2.2 Scale Setup

Move the scale into the area where the weighing process will occur. Place the scale on a hard, level surface for the most accurate weighments. Placing the scale on thin carpeting is not recommended.

2.2.1 Attaching Feet to the Scale


The 350-ADA-1 digital wheelchair scale comes with four feet that must be attached to the scale base for proper operation. The four feet are located in the parts box in the original shipping crate. Use the following steps to attach the feet to the scale.

1. Tip the scale onto it's side on a level surface so the scale base is accessible.
2. Remove the plastic packaging from the scale base.



Figure 2-9. Tipped Scale

 **CAUTION:** *When tipping the scale, be cautious of surroundings to prevent potential injuries.*

 **IMPORTANT:** *To avoid damaging the threading, ensure the feet are correctly aligned during installation.*

3. Rotate the four round feet clockwise into the scale base until finger-tight as shown in [Figure 2-10](#).

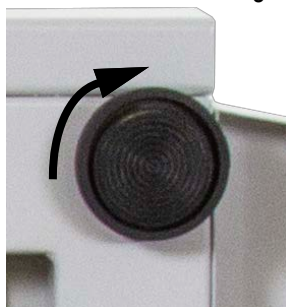


Figure 2-10. Secure Scale Platform Feet

2.2.2 Installing Ramps onto the Scale

1. Hold the ramp vertically against the end of the scale (see Figure 2-11).
2. Starting from the top, thread each of the five screws through the ramp into the scale without fully tightening.

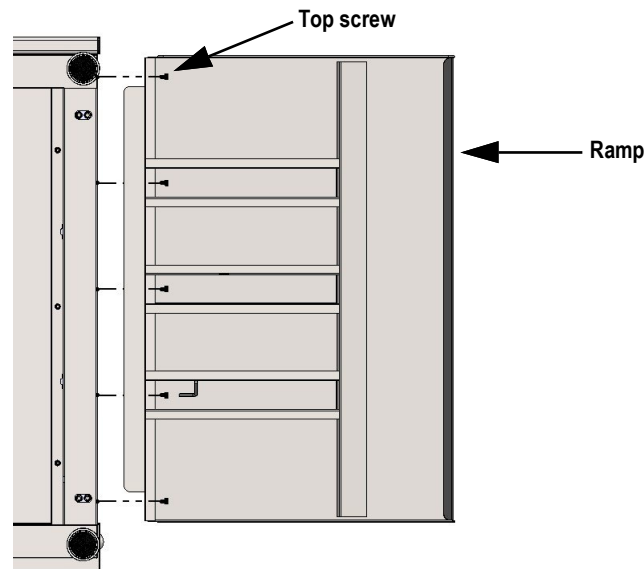


Figure 2-11. Attaching Ramp to Scale

3. Once all screws are threaded, tighten each screw with the 5 mm Allen wrench provided.

IMPORTANT: To avoid damaging the threading, ensure all screws are properly aligned before tightening.

4. Repeat Step 1 to Step 3 for the second ramp.

2.2.3 Leveling the Scale Base

CAUTION: Lowering the scale should be accomplished by two people. Do not lower the scale by the handrails. Instead, lower the scale by the scale base.

1. With assistance, gently set the scale base down on to the floor. Ensure there is minimal clearance between the scale base and the floor without having the scale base contacting the floor.



Figure 2-12. Scale Base Clearance

2. It is important to ensure that the scale is completely level. Gently press down on all corners of the scale base to ensure that there are no high spots or rocking of the scale base.
3. Adjust feet as needed to level the scale.

NOTE: An uneven base will produce inaccurate weight readings.

2.2.4 Hinge Setup

1. Remove the bubble wrapping from the handrail and indicator.
2. Loosen the knobs by rotating counterclockwise and set the scale arms upright.



Figure 2-13. Loosen the Durable Hinges to Set Handles Upright

3. Tighten the two hinges on the 350-ADA-1 digital wheelchair scale by tightening the two knobs by rotating clockwise to secure the handrail mounted indicator.

2.2.5 Insert Alkaline Batteries

The six AA batteries supplied with the scale provide an average of 25 hours of continuous use.

To install the batteries:

1. Turn thumbscrew counterclockwise then remove battery cover.
2. Insert batteries into the battery chamber as illustrated.



Figure 2-14. Battery Chamber

3. Put the cover in place and turn the thumbscrew clockwise to secure.



NOTE: Remove the batteries prior to storing if the product is not going to be used for an extended period of time.



NOTE: If the LO BAT indicator activates, for accurate weighing, replace the batteries or connect the scale to an AC power source as soon as possible.

2.2.6 Power Connection

An optional AC power adapter can be used when a power outlet is available.



IMPORTANT: Only use power adapters supplied by or purchased from Rice Lake Weighing Systems. The use of a power adapter not from Rice Lake Weighing Systems voids the warranty.

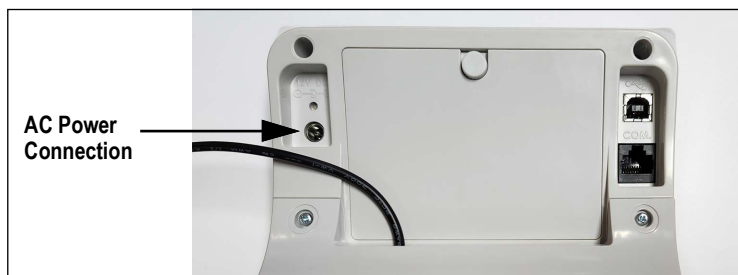


Figure 2-15. Power Connection Site



NOTE: The battery annunciator on the display turns off when using an AC power connection. The brightness of the backlight is reduced to 60% when using battery power.

3.0 Operation

This section describes the front panel and includes procedures for operation of the scale.



Figure 3-1. Front Panel Keypad

3.1 Key Descriptions

The display has 10 front panel keys. Key functions are described in the table below.

IMPORTANT: The front panel keys are very sensitive, so only a gentle press is required.














| Key | Name | Function |
|---|--------------|---|
|  On/Off | On/Off | Powers the scale on or off |
|  Print LB/KG | Print LB/KG | Sends data out from the RS-232 port; Allows to toggle between kilograms and pounds providing that it is enabled in Configuration mode; Cannot toggle while in the BMI mode |
|  Zero | Zero | Only functions if the current weight is stable and less than 2% of the capacity of the scale. Anything over 2% requires a recalibration |
|  Hold Release | Hold Release | Displays most current weight value on the display and holds that value when the patient is off the scale. A second press releases the weight value. Not active while in BMI mode |
|  BMI | BMI | Pressing the BMI key enables access to the BMI (Body Mass Index) mode (defaults when scale is turned on). The patient is gets on the scale, weight stabilizes and press the BMI key. The display then asks for the patient height to calculate out the patient BMI. |
|  TARE | TARE | Used to remove the weight initially of anything on the scale that shouldn't be included in the total weight of the patient on the scale |
|  CLEAR | CLEAR | When using the BMI function, the display looks for a height entry. Pressing Clear changes this entry back to 190.0 cm (default) or 5 ft, 7.5 in. Once BMI is displayed, pressing the Clear key exits BMI |
|  ENTER | ENTER | Used to accept height in BMI mode; accepts the value of the parameter last entered and moves to the next stage. Pressing and holding Enter during startup will display ID. This is the first setup on entering into configuration mode |
|  Up Arrows | Up Arrows | Adjusts the value of the flashing digit/number Adjusts height input (0.5 in/0.5 cm) while in BMI mode |
|  Down Arrows | Down Arrows | Adjusts the value of the flashing digit/number Adjusts height input (0.5 in/0.5 cm) while in BMI mode |

Table 3-1. Key Functions




3.2 Weighing

Use the following steps to weigh.

1. Press  to turn on the scale. **0.0** appears on the display along with the **ZERO** annunciator.
2. Place the patient on the scale. The patient's weight is displayed, the **LOCK** annunciator is on and the indicator beeps to indicate the end of the weighing process.
3. Press  to change the display from lb to kg and vice-versa.
4. Press and hold  until **OFF** displays to turn off the scale.

3.3 Hold/Release Function

Use the following steps to use the Hold/Release function.

1. Press  to turn on the scale. **0.0** prompts along with **ZERO** on the display.
2. Press  once the patient's weight stabilizes. The patient's weight and the **HOLD** and **LOCK** annunciators remain on the display when the patient is off the scale.
3. Press  again to return the scale to zero.





NOTE: Pressing  will not work while using Hold/Release function.



NOTE: Pressing  prior to the patient getting on the scale will also hold the weight display.


3.4 Preset Tare

Use the following steps for the Preset Tare function prior to patient weighing if additional items are being used by the patient.

1. Press  to turn on the scale. **0.0** appears on the display along with the **ZERO** annunciator.
2. Place additional item(s) on the scale.
3. Press  until the display returns to **0.0** and **NET** annunciator appears on the display.
4. Remove additional item(s) from the scale. The weight displays with a negative symbol to the left of it.



NOTE: Not removing the additional item(s) prior to patient weighing will also work.





5. Position the patient and additional item(s) on the scale. The display identifies the patient weight. The **NET** annunciator is still active. The weight of the additional item(s) remains stored in memory for the duration of this weigh in.
6. To cancel the tare weight, remove patient from the scale and press  until **NET** disappears from the display and the display turns back to **0.0** and **GROSS** appears.



NOTE: Tare weight is also canceled when the scale is turned off.

3.5 Toggle Tare






Use the following steps to use the Toggle Tare function when the additional item to be weighed is known.

1. Press  when the scale is empty and **0.0** displays. The default values prompts while **0.0** is flashing on the display (default is programmed to be 33.0 lb/15.0 kg).
2. Use  and  to adjust the value. Press  to start the tare function. The **NET** annunciator turns on instead of the **GROSS** annunciator.






3.6 Using the Body Mass Index (BMI) Function

Use the following steps in determining the BMI.

3.6.1 LB Mode

1. Ensure that the scale is at zero.
2. Place the patient on the scale to obtain a weight. The **LOCK** annunciator appears on the display.
3. Press . The **BMI** and **FT/IN** annunciators appear on the display and a default height value of 5 feet - 7.5 inch (5 - 07.5) is flashing.
4. Use  and  to adjust the height value.
5. Press .
6. The BMI value and **BMI** annunciator are shown on the display. Press  to return to the **Weighing** mode and the BMI function will be turned off.

3.6.2 KG Mode

1. Ensure that the scale is at zero.
2. Place the patient on the scale to obtain a weight. The **LOCK** annunciator appears on the display.
3. Press . The **BMI** and **CM** annunciators appear on the display and a default height value of 170.0 cm (170.0) is flashing.
4. Use  and  to adjust the height value.
5. Press .
6. The BMI value and **BMI** annunciator are shown on the display. Press  to return to the **Weighing** mode and the BMI function will be turned off.

3.7 Troubleshooting

Refer to the following table to check and correct any failure before contacting service personnel.

| Symptom | Possible Cause | Corrective Action |
|--|---|---|
| Scale does not turn on | Dead batteries | Replace batteries or connect to AC power |
| | Faulty electrical outlet | Use a different electrical outlet |
| | Bad power supply | Replace adapter |
| Questionable weight or the scale does not zero | External object is interfering with the scale | Remove the interfering object from the scale |
| | Display did not show 0.0 before weighing | Help the patient off the scale, zero the scale and begin the weighing process again |
| | Scale is not placed on a level floor | Ensure scale is level and begin the weighing process again |
| | Scale is out of calibration | Check the weight with a certified calibration weight |
| | Scale base is touching floor during a weighment | Adjust height of feet so fingers can slide between the base of scale and the floor all the way around the platform |
| The display shows a STOP message | The load on the scale exceeds the capacity of the scale | Remove the excess weight and use the scale according to manufacture specifications |
| The display shows LO Bat message | The battery is low | Replace batteries |
| The display shows E and Err messages as detailed below | | |
| E06 | Identifier - ADC | AD too high |
| E07 | | AD too low |
| E10 | Overload | Scale has been overloaded. Remove load from scale |
| E4L | BAT | Battery low, but still usable- one bar left on indicator display |
| E4U | | Battery low and unstable - no bars left on indicator display |
| E11 | CAL | Calibration Error - recalibrate scale |
| Err 1 | Load cell cable may be plugged into wrong connection port | Ensure cable is connected to the load cell connection port. Note: Load cell connection point is located underneath the curved plastic cover of the indicator. Remove four back retaining screws, remove curved back cover to access load cell connection point. |
| Err 2 | Low saturation state (low A/D) | The load cell is not connected properly; Check the cables and mechanical connections; if the problem persists, replace the set of load cells |
| Err 3 | High saturation state (high A/D) | See Err 2 |
| Err 6 | Unstable weight; Cannot calibrate | Check the load cell mechanical surroundings and ensure nothing is contacting the load cell and that the cables are properly welded |
| Err 7 | Scale isn't moving | Make sure feet are installed on the scale. Turn the feet all the way in and then back them out three full turns, then level the scale |
| SAT | Damaged load cell cable | Replace load cell cable |
| | Load cell cable may be plugged into wrong connection port | Ensure cable is connected to the load cell connection port. Note: Load cell connection point is located underneath the curved plastic cover of the indicator. Remove four back retaining screws, remove curved back cover to access load cell connection point. |

Table 3-2. Troubleshooting Table

4.0 Configuration

Options and parameter setup are done through the scale configuration.

4.1 Setup Switch

Access to the setup switch is located under the tilt stand cover. Use a Phillips head screwdriver to remove the four screws holding the cover in place (shown below — left photo).

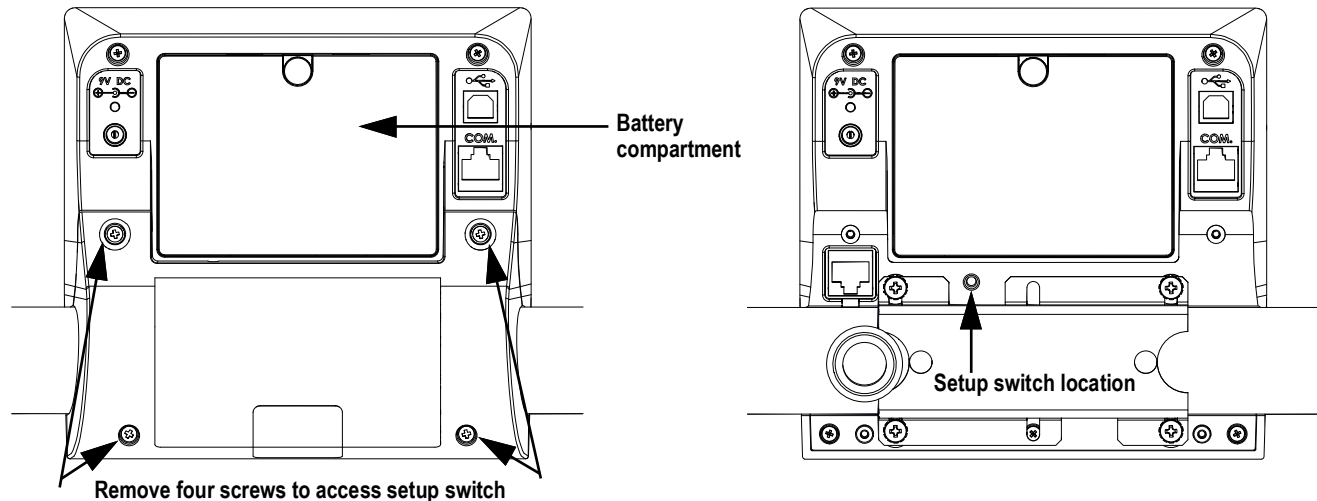


Figure 4-1. Setup Switch Location

4.2 General Navigation

Use the buttons on the front panel to navigate through the menus and parameters.

4.2.1 Change Parameters


- Press **BMI** to scroll through the menus and/or parameters
- Press **ENTER** to enter a displayed menu and/or parameter
- Press **▲** or **▼** to scroll through values
- Press **ENTER** to save the displayed selection and move to the next parameter

4.2.2 Enter Numbers

- Press **ENTER** to enter parameter value
- Press **▲** or **▼** to increment/decrement numbers
- Press **BMI** to move to the next digit
- Press **ENTER** to save value and move to the next parameter



4.2.3 Save and Return to Main Menu


- When a parameters selection/value is correct, press **ENTER**. The next parameter displays
- When all parameters selections/values are correct, **SAVE** displays
- Press **ENTER**. **DONE** displays.

- Press  to save settings and return to weigh mode.

4.3 Configuration Mode



Use the following steps to enter into **Configuration** mode.

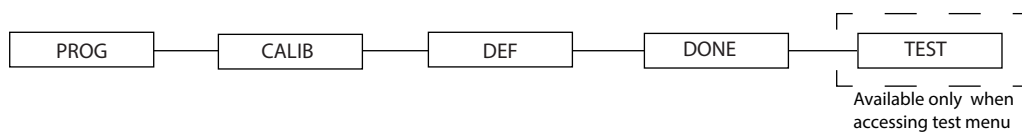1. Ensure the scale is turned off.
2. Turn the scale on by simultaneously pressing  and . Continue to hold both keys until **ld** appears. The unit cycles through its startup function and continues to display the software version.
3. Access the setup switch located in the back of the scale to enter the setup parameters for the scale. Use a small paper clip, small screwdriver or other similar object to press the setup switch.
4. Once the setup switch is pressed, **PROG** displays.
5. Scale can be configured using a series of menus accessed through the front panel when the scale is in **Setup** mode.



See [Section 4.7 on page 25](#)

Figure 4-2. Top Level Menu

6. Press  to advance to the desired menu.
7. Press  and advance in the manual to the related menu selection for further instructions.

4.4 Programming Mode Menu

Various parameters can be set while in **Programming** mode.

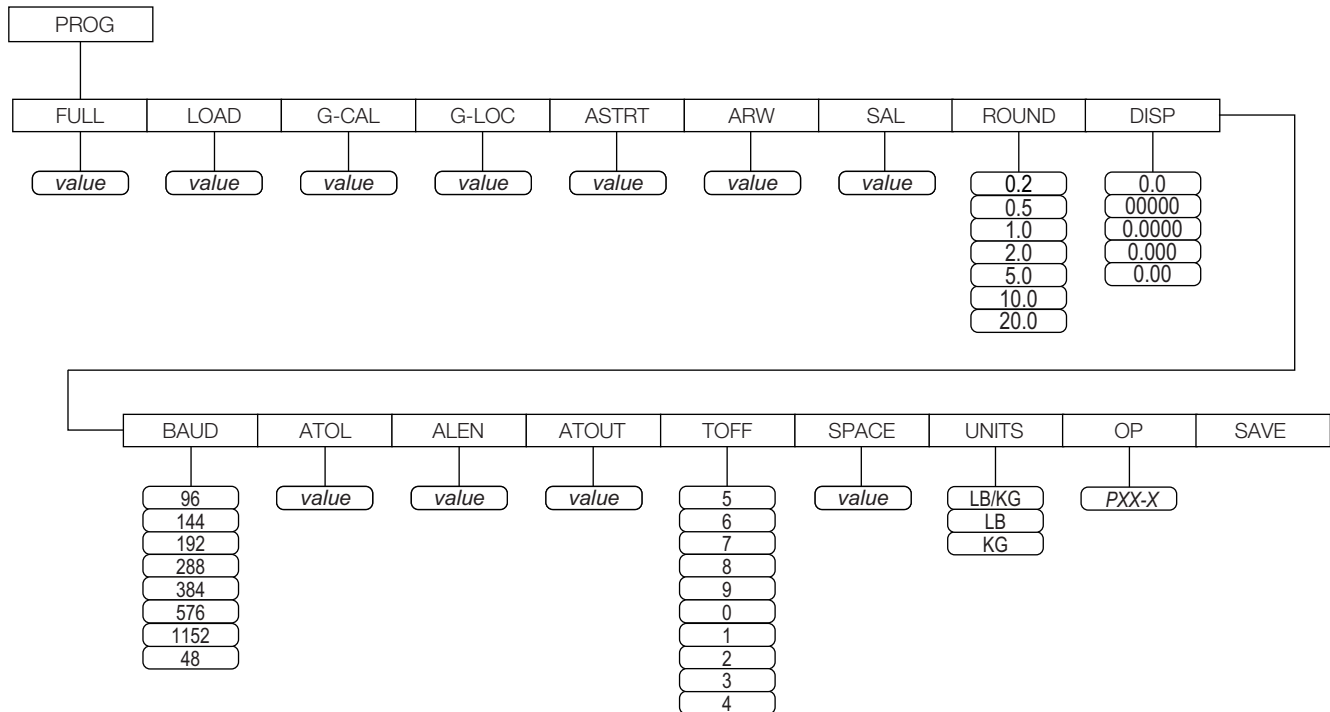


Figure 4-3. Programming Mode Menu Structure

The following table lists the various display messages and sequence when setting up the scale.

| Parameter | Description | Choices | Steps |
|-----------|--|------------------------------------|--|
| FULL | Full capacity of the scale | Value (<i>capacity of scale</i>) | The display toggles between a numeric value and FULL ; If you do not want to change the value, press the BMI key to move to the next setting; Example: from FULL to LOAD. If you want to change the value, use the following steps; 1. Press ENTER key to change value starting with the right most digit. 2. Use the Up/Down arrow keys to increment/decrement numbers. 3. Press BMI key to move to the left. 4. Use the Up/Down arrow keys to increment/decrement numbers. 5. Press BMI key again to move to the left 6. Use the Up/Down arrow keys to increment/decrement numbers. 7. When done press ENTER key to move to the next parameter (LOAD). |
| LOAD | This is the amount of weight applied during calibration; Can also be changed in the calibration menu | Value (200 lb) | The display toggles between a numeric value and LOAD ; If you do not want to change this value, press the BMI key to move to the next setting; Example: from LOAD to ASTART; If you want to change the value, use the following steps; 1. Press ENTER key to change value starting with the right most digit. 2. Use the Up/Down arrow keys to increment/decrement numbers. 3. Press BMI key to move to the left. 4. Use the Up/Down arrow keys to increment/decrement numbers. 5. When done, press ENTER key to move to next parameter (ASTART). |

Table 4-1. Configuration Mode Menu

| Parameter | Description | Choices | Steps |
|-----------|--|--|--|
| ASTART | Weight process start limit — Maximum (full capacity)/10; Determine when the weight algorithm starts (when the “----” is displayed), below this value the scale will show live weight | Value (2.0) | The display toggles between a numeric value and ASTART ; If you do not want to change this value, press the BMI key to move to the next setting; Example: from ASTART to ARW; If you want to change the value, use the following steps; 1. Press ENTER key to change value starting with the right most digit. 2. Use the Up/Down arrow keys to increment/decrement numbers. 3. Press BMI key to move to the left. 4. Use the Up/Down arrow keys to increment/decrement numbers. 5. When done, press ENTER key to move to the next parameter (ARW). |
| ARW | Auto Reweigh — Restarts the weight algorithm if the weight changed by more than this value. | Value (4.0 lb) | The display toggles between a numeric value and ARW ; If you do not want to change this value, press the BMI key to move to the next setting; Example: from ARW to SAL; If you want to change the value, use the following steps; 1. Press ENTER key to change value starting with the right most digit. 2. Use the Up/Down arrow keys to increment/decrement numbers. 3. Press BMI key to move to the left. 4. Use the Up/Down arrow keys to increment/decrement numbers. 5. When done, press ENTER key to move to the next parameter (SAL). |
| SAL | Semi Auto Live — This value is the interval between weight displays during the algorithm process | Value (0.5) | The display toggles between a numeric value and SAL ; If you do not want to change this value, press the BMI key to move to the next setting; Example: from SAL to ROUND; If you want to change the value, use the following steps; 1. Press ENTER key to change value starting with the right most digit. 2. Use the Up/Down arrow keys to increment/decrement numbers. 3. When done, press ENTER key to move to the next parameter (ROUND). |
| ROUND | Scale Resolution — Values in kg: 1, 2, 5, 10, 20, 50, 100 Values in lb: 1, 2, 5, 10, 20, 50, 100, 200 | 0.2 0.5 1.0 2.0 5.0 10.0 20.0 0.1 | The display toggles between a numeric value and ROUND ; The decimal point location is set to the DISP parameter display decimal point location; If you do not want to change this value, press the BMI key to move to the next setting; Example: from ROUND to DISP; If you want to change the value, use the following steps; 1. Press ENTER key to change value. 2. Press the Up/Down arrow keys to change the available parameters. 3. When done, press ENTER key to move to the next parameter (DISP). |
| DISP | | 0.0 0 0.0000 0.000 0.00 | The display toggles between a numeric value and DISP ; If you do not want to change this value, press the BMI key to move to the next setting; Example: from DISP to BAUD; If you want to change the value, use the following steps; 1. Press ENTER key to change value. 2. Use the Up/Down arrow keys to change the available parameters. 3. When done, press ENTER key to move to the next parameter (BAUD). |
| BAUD | Baud rate | 96 48 1152 576 384 288 192 144 | Indicator display illustrates first two digits of baud rate only; The display toggles between a numeric value and baud; If you do not want to change this value, press the BMI key to move to the next setting; Example: from BAUD to ATOL; If you want to change the value, use the following steps 1. Press ENTER key to change value. 2. Use the Up/Down arrow keys to change the available parameters. 3. When done, press ENTER key to move to the next parameter (ATOL). |
| ATOL | Algorithm initial tolerance — Maximum value is 255. Values above 255 will not let you proceed and will return to the previous value. | Value (10) | The display toggles between a numeric value and ATOL ; If you do not want to change this value, press the BMI key to move to the next setting; Example: from ATOL to ALEN; If you want to change the value, use the following steps; 1. Press ENTER key to change value starting with the right most digit. 2. Use the Up/Down arrow keys to increment/decrement numbers. 3. Press the BMI key to move to the left. 4. When done, press ENTER key to move to the next parameter (ALEN). |

Table 4-1. Configuration Mode Menu (Continued)

| Parameter | Description | Choices | Steps |
|---|---|--|--|
| ALEN | Algorithm initial exponent — Maximum value 10. Values above 10, will not let you proceed and will return to the previous value. | Value (8) | The display toggles between a numeric value and ALEN ; If you do not want to change this value, press the BMI key to move to the next setting; Example: from ALEN to ATOUT; If you want to change the value, use the following steps; 1. Press ENTER key to change value starting with the right most digit. 2. Use the Up/Down arrow keys to increment/decrement numbers. 3. When done, press ENTER key to move to the next parameter (ATOUT). |
| ATOUT | Algorithm maximal exponent — Maximum value is 15. Values above 15, will not let you proceed and will return to the previous value. | Value (10) | The display toggles between a numeric value and ATOUT ; If you do not want to change this value, press the BMI key to move to the next setting; Example: from ATOUT to TOFF; If you want to change the value, use the following steps; 1. Press ENTER key to change value starting with the right most digit. 2. Use the Up/Down arrow keys to increment/decrement numbers. 3. Press BMI key to move to the left. 4. Use the Up/Down arrow keys to increment/decrement numbers. 5. When done, press ENTER key to move to the next parameter (TOFF). |
| TOFF | Auto off timer — Measured in minutes; 0 = always on; Maximum is 9 minutes; When using an external power supply, this parameter is irrelevant | 5 4 3 2 1 0 9 8 7 6 | The display toggles between a numeric value and TOFF ; If you do not want to change this value, press the BMI key to move to the next setting; Example: from TOFF to UNITS; Press the ENTER key to move to the next parameter; (UNITS); If you want to change the value, use the following steps; 1. Press the ENTER key to change values. 2. Use the Up/Down arrow keys to change the available parameters. 3. When done, press ENTER key to move to the next parameter (UNITS). |
| UNITS | Units — Selects the unit of measure; It can be either Kg/Lb, Kg only or Lb only | KG/LB KG LB | The display toggles between unit of measurements and UNIT ; If you do not want to change this value, press the BMI key to move to the next setting; Example: from UNITS to OP; If you want to change the value, use the following steps; 1. Press the ENTER key to change values. 2. Press the Up/Down arrow keys to change the value. 3. When done, press the ENTER key to move to the next parameter (OP). |
| OP | Binary options: OP0 — Live weighing options (0=disable, 1=enable) OP1 — Communication protocol (0=ESC, 1=maintenance) OP2 — BMI menu (0=disable, 1=enable) OP3 — RTC power (0=disable, 1=enable) OP4 - Semi-Auto-Live — (0=disable, 1=enable) OP5 - Full calculation — (0=spatial, 1=multi- ply by (0=disable, 1=enable) OP6 - Tare - (0=disable, 1=enable) OP7 - Bat type — (0=dry batteries, 1=rechargeable batteries) OP8 — OIML mode - (0=disable, 1=enable | OP0 OP1 OP2 OP3 | The display toggles between a binary option and POO-0 ; If you do not want to change this value, press the BMI key to move to the next settings If you want to change the value, use the following step 1. Press ENTER to change parameters. 2. Use the Up/Down arrow keys to select the display value you want to change. 3. Press BMI key to move the flashing cursor a. Use the Up/Down arrows to change the value. b. Press the BMI key to move the flashing cursor. 4. Press ENTER key to save all of the display parameters. SAVE appears on the display. 5. Press ENTER key again and DONE appears indicating that you are now done entering all of the parameters of the scale. |
| Press the BMI key to cycle back to the top level menu choices, ie: PROG/CALIB/DEF/DONE | | | |

Table 4-1. Configuration Mode Menu (Continued)

4.5 Default Menu

The default menu is used to return the scale back to its factory settings and is shown below.

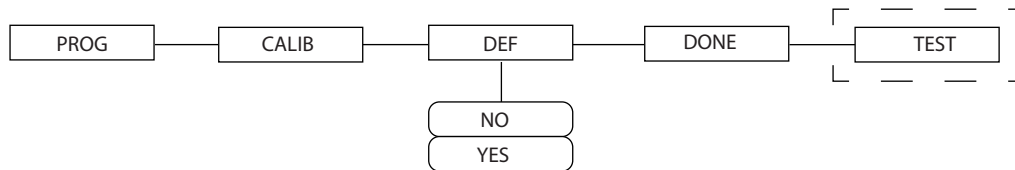


Figure 4-4. Default Menu

Use the following steps to return the settings back to their factory default.

1. Press . The display shows a default value of **NO**.
2. To change to **YES**, use and to adjust the value.
3. Press and the display shows **DONE**.
4. Press to return to top level level menu.








NOTE: Selecting **YES** and pressing will reset to factory defaults settings without changing the calibration and will return you to Weigh mode.

4.6 Scale Calibration







Use the following steps to calibrate the scale.

1. Press and simultaneously to power on the scale.
2. The unit cycles through its startup function and continues to display the software version. Continue to hold both keys until **ld** appears.
3. Access the setup switch located in the back of the scale to enter the setup parameters for the scale. Use a small paper clip, small screwdriver or other similar object to press the setup switch on the back of the indicator (under the cover).
4. **Prog** displays. Press to toggle along the parameter menu.
5. **Calib** displays and enter the calibration parameters.
6. Press and a numeric value is displayed which represents the amount of weight that is used for calibration.
Lb will be flashing. To switch between lb and kg, press or . Once a unit is selected, press and the right most digit will be flashing.
7. To change the calibration load value, press or to increment/decrement the flashing digit.
8. Use to move the flashing digit to the left or right.
9. Once all the digits have been entered, press and **Clear** displays.
10. Make sure the scale platform is clear of weight and press again then ===== displays.
11. A request to put the chosen load on the platform is displayed by **Put xxx.xx**.
12. Put the chosen weight on the platform and press . ===== displays then **Save** displays.

13. Press  again and the display indicates **Done**.
14. Press  three times to exit back out to the top level **Done** parameter.
15. Press  to return to **Weigh** mode.
16. To exit calibration without changing zero or span existing calibration, press , then press .

4.7 Test Menu

To access the **TEST** menu, use the following steps.

1. Press  and  simultaneously to power on the scale until **ID** flashes.
2. Press  again.
3. Continue to press  to scroll through the various menu items.
4. Once complete, press  again then **Done** displays.
5. Press  to start the weighing process.

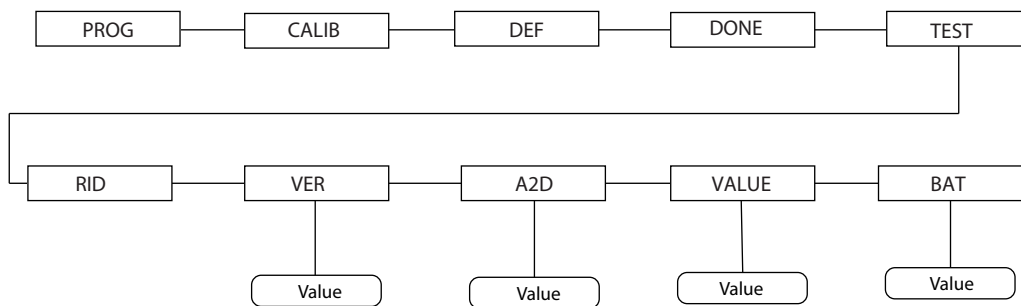


Figure 4-5. Test Menu

| Parameter | Choice | Description |
|-----------|--------|---|
| RID | Value | Displays internal ID number |
| VER | Value | Displays the current software version |
| BAT | Value | Displays the current battery level |
| VALUE | Value | Displays the actual value |
| A2D | Value | Displays the actual raw counts of the scale |

Table 4-2. Test Menu

5.0 Communication

The unit comes with an RS-232 port that enables weight data to be transmitted to other equipment, such as a computer or printer. The RS-232 cable with DB-9 connector (PN 100719) is available from Rice Lake Weighing Systems. That connection is shown in USB Connection section.


The RS-232 parameters are:

- 9600 baud (selectable in the programming mode)
- 8 data bits
- 1 stop bit
- no parity
- no handshaking

There are three methods of communication:

- Push-button keypad print
- Standard remote protocol
- Escape protocol

5.1 Push-button Keypad Print

With a stable, in-range weight, press and hold  for at least three seconds, or until the scale emits two quick beeps.



NOTE: If the scale does not beep after five seconds, release  as the weight was either in motion or out of range.

If displaying weight and not BMI, the scale will send out the following 21 character string:

```
xxxxxxxx<SP>uu<SP>mmmm<SP><CR><LF>
```

| Token | Description |
|----------|--|
| xxxxxxxx | Weight with decimal point and “-” sign |
| <SP> | Space |
| uu | Unit - lb or kg |
| mmmm | Mode - gross or net |
| <CR> | Carriage return |
| <LF> | Line feed (moves cursor down to the next line) |

Table 5-1. Print Format Tokens

Example:

```
60.1 KG= <PATIENT><SP><WEIGHT><SP>-60.1<SP>KG<SP><CR><LF>
```

In BMI mode (displaying the BMI value), the scale will send out the following data:

```
PATIENT WEIGHT    60.1 KG
PATIENT HEIGHT 170.0 CM
PATIENT BMI       20.8
```

Example in KG:

```
<PATIENT><SP><WEIGHT><SP>-60.1<SP>KG<SP><CR><LF>
<PATIENT><SP><HEIGHT><SP>-170.0<SP>CM<SP><CR><LF>
<PATIENT><SP><B><SP><M><SP><I><SP><SP><SP><20.8<SP><SP><SP><CR><LF>
```

Example in LB:

```
<PATIENT><SP><WEIGHT><SP>132.4<SP>LB<SP><CR><LF>
<PATIENT><SP><HEIGHT><SP>5-07.5<SP>FT<SP><CR><LF>
<PATIENT><SP><B><SP><M><SP><I><SP><SP><SP><20.4<SP><SP><SP><CR><LF>
```

In case of under weight or over weight, the word **Under** or **Over** will be sent correspondingly.

5.2 Communication Protocols

The scale has two communication protocols, escape and maintenance protocol.

5.2.1 Escape Protocol

An escape protocol is where the escape (0X1B or ASCII 27) is used to indicate that there is a command following. On the PC side there must be a listener created by the vendor that will interpret this protocol. This listener must also take care of all the issues regarding data integrity to make sure that the data that was sent and received is valid.

Two examples include:

- Scale initiated communication
- PC initiated communication

The escape protocol commands table shows (below) what can be sent across communications lines.

| PC Initiated | ESC Value |
|---------------------------------|-----------|
| Request current values/settings | R |
| Diagnostics | A |
| Send scale control messages | C |
| PC Initiated | ESC Value |
| Send single reading | R |
| Send diagnostic response | |

Table 5-2. Escape Protocol Commands

ESC characters that will be used is shown below.

| Name | ESC Character | ESC Value with Parameters | Description |
|------------------------|---------------|---------------------------|--|
| Reading | R | R | Tells PC the scale is sending a reading; immediately following this is the value that is sent Example: <ESC><R>ESC><W0200.0<ESC>Nm<ESC>E |
| Weight | W | Wnnn.n | The patient weight (<i>Example: W02000 means 200.0</i>). If scale is overloaded or under loaded, 999.99 is returned |
| Height | H | Hnnn.n | Patient height |
| BMI | B | Bnn.n | Patient BMI |
| Units | N | Nc | Indicates the units the values have been taken (<i>m=metric, c=constitutional</i>). |
| End of Packet (EOP) | E | E | Indicates the end of the command has been reached. |
| Diagnostics (request) | A | Accc | A request for a diagnostic test on certain parts of the scale (like battery life, load cells). |
| Diagnostics (response) | Z | Zccc | The response of the diagnostics done on the scale; values include error codes to indicate an issue, or all zeros (Z000) to indicate the scale is performing properly |
| Control (set a value) | C | Cccc=c | Sets the value of the scale's global settings <i>Example: <ESC><CUOM=m><ESC><E sets the unit of measurement</i> |

Table 5-3. ESC Characters

| Name of Control | Identifier | Unit |
|--|------------|------------|
| Unit of Measure (metric or constitutional) | UOM | c (m or c) |

Table 5-4. Scale Global Values and Identifiers

Samples of Escape Protocol

Examples of what is sent to the computer from the scale.

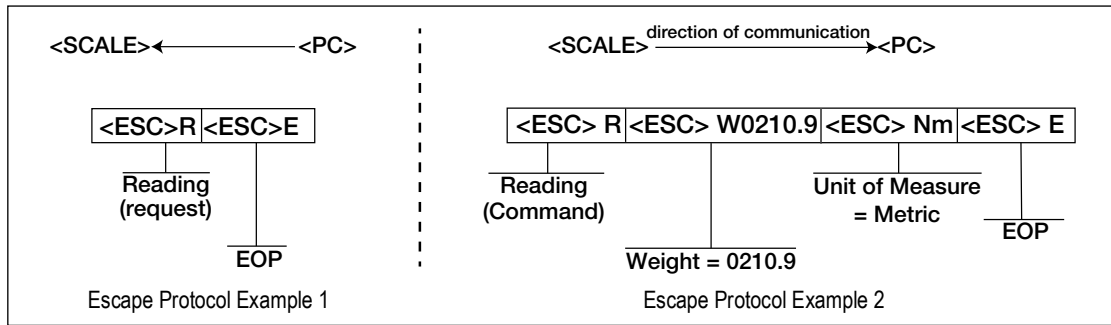


Figure 5-1. Escape Protocol Examples

Examples of diagnosing battery request and responses.

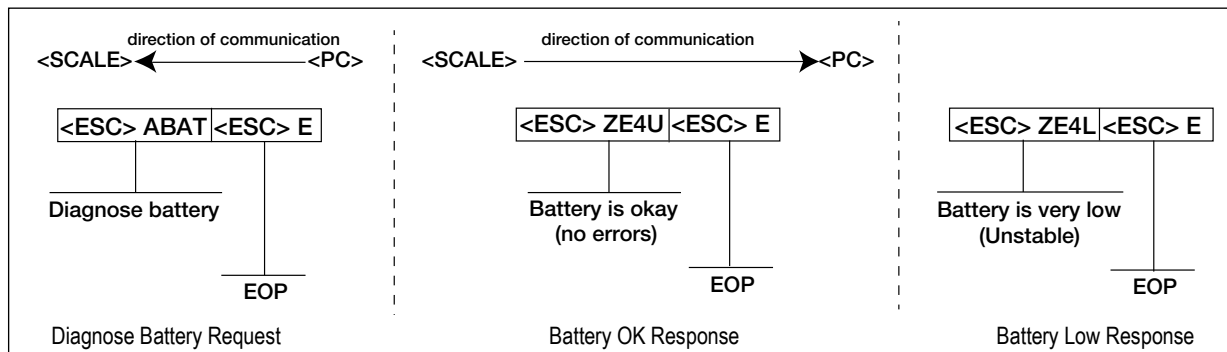


Figure 5-2. Diagnose Battery Examples

5.2.2 Maintenance Protocol

Maintenance protocol commands are listed below.

| Command | Definition |
|---------|--|
| R | Reboot |
| V | Firmware ID + development version |
| W | Current weight |
| A | Current AD |
| Z | Zero the scale |
| F | Show flash values (used for the first flash process) |
| L | USB On/Off (not available on USB communication) |

Table 5-5. Maintenance Protocol Commands

5.3 USB Connection

The scale has the capability of connecting to a Windows® computer (PC) using a USB cable (not included) and a terminal emulation program. A terminal emulation program allows the transfer of data between the scale and PC using a serial port.



Figure 5-3. Connection Ports

NOTE: Apple® and Macintosh® computers are unable to transfer the necessary data to the scale. Only use a PC for data transfer.

Connecting software and downloads should always be addressed by the IT department for safety reasons and can vary depending on what type of computer platform is being used.

NOTE: Consult the IT department if driver protections are preventing the use of the USB driver. Driver protections may need to be temporarily disabled on Windows 10 or later computers to allow for the installation of the USB driver.

1. Connect the scale's indicator to a PC using a USB-Type B to USB-Type A cable (not included).
2. Turn the indicator on.

NOTE: In most cases, the PC should find the driver and automatically configure the driver when the scale is plugged into a USB port.

3. Open a terminal emulation program, such as Advanced Serial Port Terminal, pUttY or Hercules (used in this example).
4. Connect to the serial port assigned by the PC (COM5 in example). This can be found in Device Manager. Once selected, press **Open**.

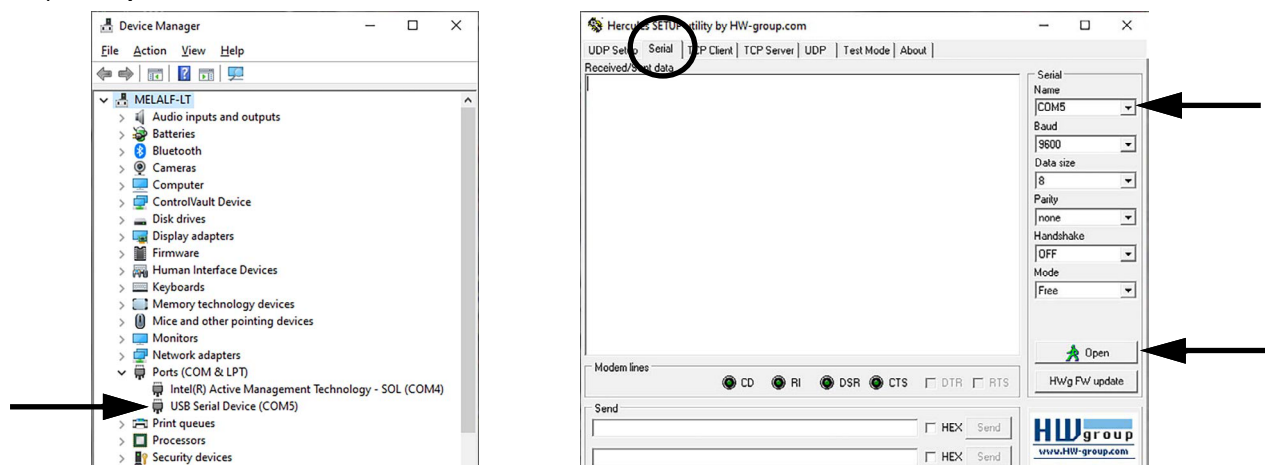


Figure 5-4. Connecting to a Serial Port

5. With weight on the scale, press and hold the **Print** button on the indicator for three seconds. The patient's weight is sent to the PC.

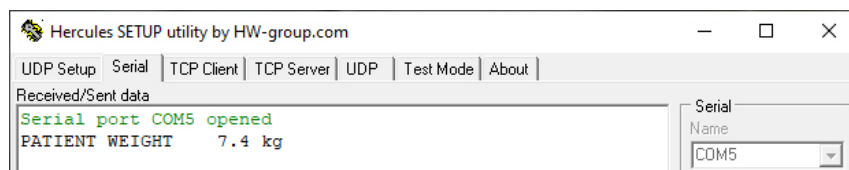


Figure 5-5. Patient Weight Displayed

6.0 Maintenance

The following section provides instructions for maintaining and cleaning the unit.



IMPORTANT: Do not immerse the scale in cleaning or other liquid solutions.

Do not use Isopropyl alcohol or other solutions to clean the indicator display surface.

6.1 Basic Maintenance

Before the first use of the scale and after periods of non-use, check the scale for proper operation and function. If the scale does not operate correctly, contact a qualified service personnel.

Go through the following steps for basic maintenance.

- Check the overall appearance of the entire scale for any obvious signs of damage
- Inspect the condition of the AC power adapter cord for cracking, fraying or for broken or bent prongs

6.2 Cleaning

Proper care and cleaning is essential to ensure a long life of accurate and effective operation. Before beginning the cleaning process, disconnect the scale from the AC power source.

- Clean all external surfaces with a clean, damp cloth or tissue. Mild soap and water solution may be used. Dry with a clean soft cloth
- Do not immerse the scale into cleaning or other liquid solutions
- Do not use Isopropyl alcohol or other solutions to clean the display surface

6.3 Periodic Maintenance

Refer to the following table for periodic maintenance guidelines:

| Task | Process | Daily/Weekly | Quarterly | Per Local Regulations |
|---------------------------------|--|--------------|-----------|-----------------------|
| Routine Cleaning | Remove dirt, dust and debris | X | | |
| Ensure scale is level | Check level and adjust scale feet as needed | X | | |
| Test repeatability and accuracy | Place a minimum of 5% of full scale capacity on the scale 3 times in each quadrant | | X | |
| Inspect for damage | Check AC power adapter, hinges, etc for visible damage or missing parts | | X | |
| Calibrate | Perform certified calibration | | | X |
| Certification | Review and renew test weight certifications | | | X |

Table 6-1. Periodic Maintenance

7.0 Specifications

Power

120 VAC - 9 VDC - 60Hz / 230 VAC - 9 VDC - 50Hz

Battery Type

6 AA size Alkaline batteries

Battery Use

25 hours continuous use

Automatic power-off can be configured

Data Communications

RS-232 with RJ-45 jack

USB Connection

Selectable baud rate, default - 9600

8 bits

No parity

1 stop bit

No handshaking

Environmental

Operating Temperature 50°F to 104°F (10°C to 40°C)

Storage Temperature 32°F to 122°F (0°C to 50°C)

Humidity 85% relative humidity

Capacity and Graduation

1000 lb x 0.2 lb (453 kg x 0.1 kg)

Dimensions

Platform Dimensions 40.60 in L x 32.00 in W x 4.50 in H

Platform Dimensions (incl. Handrail) 40.60 in L x 32.00 in W x 35.90 in H