

INSTRUCTIONS FOR USE

SD2^{III}

Handheld Doppler



793326-05

2026-03

HUNTLEIGH

A MEMBER OF THE ARJO FAMILY

Contents

- 1. Introduction**
 - 1.1 Unpacking / Preliminary Checks**
- 2. Safety**
 - 2.1 Warnings**
 - 2.2 Patient Applied Parts**
 - 2.3 Intended Use & Indications**
 - 2.4 Contraindications**
 - 2.5 Patient Population**
- 3. Warranty & Service**
 - 3.1 Service Life**
 - 3.2 Maintenance and Repair**
- 4. Product Identification**
 - 4.1 Product Controls**
 - 4.2 Symbol Identification**
- 5. Prepare the Doppler for Use**
 - 5.1 Battery Insertion / Replacement**
 - 5.2 Probe Connection**
- 6. Operation**
 - 6.1 Battery Saver**
 - 6.2 After Use**
- 7. Care and Cleaning**
 - 7.1 General Care**
 - 7.2 Cleaning and Disinfecting the Doppler**
 - 7.3 Cleaning and Disinfecting Probes**
- 8. Specifications**
 - 8.1 Equipment Classification**
 - 8.2 Vascular Doppler Performance**
 - 8.3 General**
 - 8.4 Environmental**
 - 8.5 Standards Compliance**
 - 8.6 Accessories**
- 9. Electromagnetic Compatibility**

1. Introduction

The SD2 is a battery powered hand-held bi-directional vascular Doppler. It provides an audible sound and visual indication of vascular bloodflow. This equipment is for use only by suitably qualified healthcare practitioners and is not intended for use by the patient.

Before using this equipment, study this manual carefully and familiarise yourself with the controls, display features and operation.

Experience with use of ultrasonic dopplers is preferable, but for novice users training material is provided with the online documents. Exposure to ultrasound should be kept As Low As Reasonably Achievable - (ALARA guidelines).

Scan the QR code on the rear cover of this IFU with a smartphone, or visit the Huntleigh website for electronic copies of user literature. All documents are available to download as PDF files. To read them, you must have a PDF reader installed on your device. Alternatively paper copies are available upon request.

1.1 Unpacking / Preliminary Checks

On receipt of your Doppler, check that all items are present and undamaged. If items are missing or have been damaged in transit, inform Huntleigh Healthcare immediately.

Handheld Doppler	IFU (this document)	Batteries
Ultrasound Gel	Carry bag	

2. Safety

2.1 Warnings

- Dopplers are screening tools to aid the healthcare professional. If there is doubt as to vascular status, further investigations should be undertaken immediately using alternative techniques.
- Do not use in the presence of flammable gases.
- Do not use in a sterile field* unless additional barrier precautions are taken.
- Do not sterilise the product or its accessories*. The product will be damaged.
- Do not expose to excessive heat, including prolonged exposure to sunlight.
- Do not dispose of batteries in fire as this can cause them to explode.
- The Doppler is not waterproof and must not be immersed.
- This product contains sensitive electronics, which are susceptible to interference, this will be indicated by unusual sounds.
- This equipment must not be modified.

*Note: *Does not apply to Intraoperative Probe. Refer to Intraoperative Probe IFU for details on cleaning/sterilisation processes.*

2.2 Patient Applied Parts

As defined in IEC 60601-1 the patient applied parts of the Dopplers are the ultrasound probes.

2.3 Intended Use & Indications

The Doppler is intended for use by qualified healthcare practitioners in primary, acute and community healthcare environments, for the assessment of vascular blood flow, to assist in diagnosis.

The Doppler is indicated for the assessment of blood flow and direction, within veins and arteries, by audible and visual means.

2.4 Contraindications

- Do not use on broken or fragile skin.
- Do not use on the eye.

2.5 Patient Population

The SD2 is suitable for use on all patient populations.

3. Warranty & Service

Huntleigh Healthcare Diagnostic Products Division standard terms and conditions apply to all sales. A copy is available on request. These contain full details of warranty terms and do not limit the statutory rights of the consumer.

Service Returns: To return the Doppler:

- Clean the product following the instructions in this manual.
- Pack it in suitable packing.
- Attach a decontamination certificate (or other statement declaring that the product has been cleaned) to the outside of the package. (Huntleigh Healthcare Ltd reserve the right to return product that does not contain a decontamination certificate).
- Mark the package 'Service Department'.

3.1 Service Life

This is defined as the period during which the device is expected to remain safe and suitable to meet its intended use, and all risk control measures remain effective.

The service life for this device is seven years.

3.2 Maintenance and Repair

There are no user serviceable parts inside the Doppler unit or probes. This product does not require periodic maintenance. Inspection is recommended each time the product is used, paying particular attention to the tip of the probes, checking for cracks etc., and to the cable and connector. Any unusual sounds or intermittent behaviour should be investigated.


Spare parts are available. Please refer to service manual for further information and part numbers. A full technical description is provided in the Service Manual 793329.

Caution


Servicing cannot be carried out while the Doppler is in use.

4. Product Identification

4.1 Product Controls

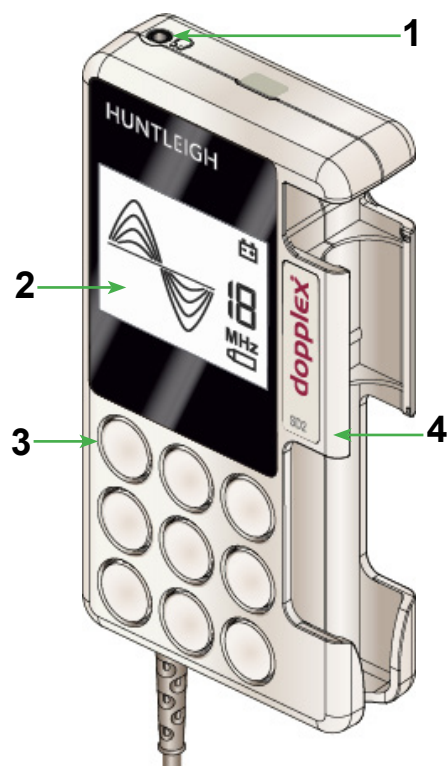

1	Headphone Socket
2	LCD Panel
3	Loudspeaker
4	Probe Holder
5	Trolley Mount
6	On/Off/Volume
7	Pocket Clip
8	Battery Compartment
9	Rear Panel Label

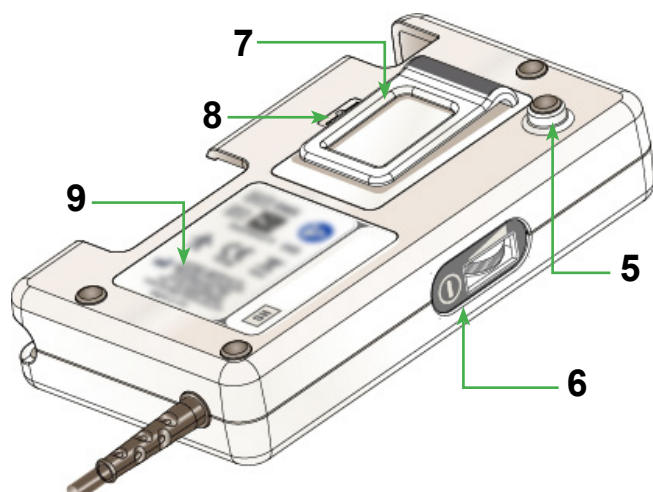

4.2 Symbol Identification

	Applied parts are type CF*		Applied parts are type BF*
	General Warning		Attention, consult accompanying documents / Instructions for Use
	This symbol signifies that this product, including its accessories and consumables is subject to the WEEE (Waste Electrical and Electronic Equipment) regulations and should be disposed of responsibly in accordance with local procedures.		
 2797	This symbol signifies that this product complies with the essential requirements of the Medical Device Directive (93/42/EEC) - Medical Device Regulation (EU/2017/745).		
RxOnly	Federal law restricts this device to sale by, or on the order of a licensed healthcare practitioner.		
	Legal Manufacturer in association with the CE mark in Europe ArjoHuntleigh AB Hans Michelsensgatan 10 211 20 Malmö, Sweden		
IP20	Protected against ingress of solid foreign objects >12.5 mm diameter. Not protected against ingress of water.		
IPx1	Protected against vertically falling water drops.		
	Power On/Off		Battery
	Device Identifier		Serial Number
	Reference Number		Medical Device
	Fragile		Keep Dry
	Atmospheric Pressure Limitations		Relative Humidity Limitations
	Temperature Limitations		Cardboard packaging can be recycled
	LATEX FREE Does not contain Latex		PVC FREE Does not contain PVC
	Headphone Socket		Volume


Note: Product labelling should be readable from a distance of up to 0.7m.

*As defined by IEC60601-1


5. Prepare the Doppler for Use

5.1 Battery Insertion / Replacement

Disconnect the Doppler from other equipment before removing the battery cover.



Insert a suitable tool into the recess, release the clip and gently lever off the battery cover.

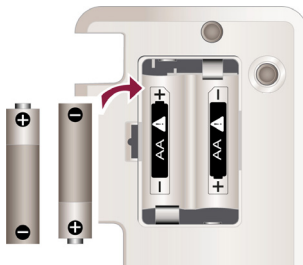

Insert the batteries according to the diagram, observing polarity.

- Use only alkaline LR6 (AA) non-rechargeable batteries.

Note: If the Doppler will not be used for an extended period, remove the batteries.

Low Battery Indication

When the batteries become depleted, a flashing battery symbol  will appear on the display. The batteries should then be replaced for reliable operation.

5.2 Probe Connection

To connect the probe, align the arrow on the connector with the slot on the probe and push together firmly.



To disconnect the probe, pull the connector from the probe. DO NOT pull the cable.

The following probe types are available:

VP4XS	4 MHz $\pm$ 1% for deep lying vessels	VP8XS	8 MHz $\pm$ 1% for peripheral vessels
VP5XS	5 MHz $\pm$ 1% for deep lying vessels and oedematous limbs	EZ8XS	8 MHz $\pm$ 1% "Widebeam" for peripheral vessels.
VP10XS	10 MHz $\pm$ 1% for specialist superficial applications.	PA8-HG	Intraoperative Probe adaptor

6. Operation

Turn the On/Off/Volume control to the On position.

Bi-directional blood flow rate and direction are indicated by the waveform displays (4 levels in each direction) along with the Probe frequency. Blood flow is audible in the loudspeaker.

Clinical Use

Apply a liberal amount of gel on the site to be examined. Place the probe at 45° to the skin surface over the vessel to be examined. Adjust the position of the probe to obtain the loudest audio signal. High pitched pulsatile sounds are emitted from arteries while veins emit a non-pulsatile sound similar to a rushing wind. After the optimum position has been found, keep the probe as still as possible. Adjust audio volume as required.

6.1 Battery Saver

To prolong battery life, the Doppler will automatically go to sleep after three minutes of no signal or ten minutes of use. To wake the Doppler, turn the On/Off/Volume control to the Off position, then On again.

6.2 After Use

Turn the On/Off/Volume control to the Off position.

Refer to the cleaning section before storing or using the unit on another patient.

7. Care and Cleaning

7.1 General Care

The Doppler contains delicate components, for example the probe tip, which should be handled and treated with care. Periodically, and whenever the integrity of the system is in doubt, carry out a check of all functions as described in the relevant section of this IFU. If there are any defects, contact Huntleigh or your distributor for repair or to order a replacement.

Caution

- Check with your facility's local infection control policy and medical equipment cleaning procedures.
- Observe warnings and guidance on cleaning fluid labelling regarding use and personal protective equipment (PPE).
- If detergent or disinfectant wipes are used, make sure that excess solution is squeezed from the wipe prior to use.
- Always switch off the Doppler and disconnect from other equipment before cleaning and disinfecting.
- Always wipe off disinfectant using a cloth dampened with clean water.
- Do not allow any fluid to enter the products and do not immerse in any solution.
- Do not use abrasive cloths or cleaners.
- Do not use automatic washers or autoclaves.
- Do not use Phenolic detergent based disinfectants, solutions containing cationic surfactants, ammonia based compounds or perfumes and antiseptic solutions.

7.2 Cleaning and Disinfecting the Doppler

Always keep the external surfaces clean and free of dirt and fluids using a clean dry cloth.

- Wipe any fluids from the surface of the product using a clean dry cloth.
- Wipe with a cloth dampened in 70% Isopropyl Alcohol.
- Completely dry with a clean, dry cloth.
- If the product has been contaminated use the methods described for probes.

7.3 Cleaning and Disinfecting Probes

(Does not apply to Intraoperative Probe IOP8/DIOP8. Refer to Intraoperative Probe IFU for details about cleaning/sterilisation processes).

Clean the probes before examining a patient using the low risk cleaning method below. Following patient examination, clean and/or disinfect the probes by the appropriate method based upon the level of cross contamination risk, as defined below:

Risk	Definitions	Procedure
Low	Normal use or low risk situations include patients having intact skin and no known infection.	1. Remove soiling, wipe with a mild neutral detergent and then wipe with a cloth dampened in water. 2. Completely dry with a clean cloth.
Medium	The patient has a known infection, skin is not intact, the part is heavily soiled.	1. Follow low risk procedure then wipe with a cloth dampened in Sodium Hypochlorite (1,000ppm). 2. After two minutes wipe with a cloth dampened in water and then dry with a clean cloth.
High	This procedure should only be used when the part has been contaminated by blood.	1. Follow low risk procedure then wipe with a cloth dampened in Sodium Hypochlorite (10,000ppm). 2. After two minutes wipe with a cloth dampened in water and then dry with a clean cloth.

Caution

Repeated and unnecessary use of concentrated solutions will result in damage to the product. Do not allow Sodium Hypochlorite solutions to come into contact with metal parts.

The use of disinfectant materials other than those listed is the responsibility of the user for their efficacy and compatibility with the device.

8. Specifications

8.1 Equipment Classification

Type of protection against electric shock	Internally powered equipment		
Degree of protection against electric shock 	 Type BF - equipment with an applied part	 Type CF - equipment connected to PA8HG/DIOP8 applied part	
Mode of operation.	Continuous		
Degree of protection against harmful ingress of particles and/or water.	Main Unit: IP20*, Probes : IPX1		
Degree of safety of application in the presence of a flammable anaesthetic	Equipment not suitable for use in the presence of a FLAMMABLE ANAESTHETIC MIXTURE WITH AIR, OXYGEN OR NITROUS OXIDE		

*For home use, this can be upgraded to IPX2 when using the protective pouch (ACC-OBS-080).

8.2 Vascular Doppler Performance

Doppler bandwidth (+0; -3 dB)			
VP4XS, VP5XS	170 to 4,600 Hz	VP10XS	270 to 8,000 Hz
VP8XS, EZ8XS	270 to 6,000 Hz	IOP8/DIOP8	110 to 7,400 Hz

8.3 General

Max. Audio Output	500mW rms typical (loudspeaker)		
Auto shut-off	After three minutes of no signal or ten minutes of use		
Headphone output	Max. output Power: 25 mW rms (32 Ω) Connector: 3.5 mm stereo jack socket		
Battery Type and Life	LR6 (AA) Alkaline cells x 2, Typically 500 one minute examinations		
Size	140 x 33 x 75 mm	Weight	294 g (without probe)

8.4 Environmental

Operating	
Temperature range	+5°C to +40°C
Relative Humidity	15% to 90% (non condensing)
Pressure	700 hPa to 1060 hPa
Transport and Storage between uses	
Without relative humidity control	-25°C to +5°C
At a r.h. of up to 90% non-condensing	+5°C to +35°C
At a water vapour pressure up to 50 hPa	>+35°C to +70°C

8.5 Standards Compliance

IEC 60601-1	IEC 60601-1-11
IEC 60601-2-37 Thermal Indices (TI) and Mechanical Index (MI) are below 0.7 for all device settings.	IEC 60601-1-2

8.6 Accessories

Use only the recommended accessories.

9. Electromagnetic Compatibility

Make sure the environment in which the Doppler is installed is not subject to strong sources of electromagnetic interference (e.g. radio transmitters, mobile phones). If not installed and used properly, in strict accordance with the manufacturer’s instructions, it may cause or be subject to interference. Type-tested in a fully configured system, complies with IEC 60601-1-2, the standard intended to provide reasonable protection against such interference. Whether the equipment causes interference may be determined by turning the equipment off and on. If it does cause or is affected by interference, one or more of the following measures may correct the interference:

- Reorient the equipment
- Relocate the equipment with respect to the source of interference
- Move the equipment away from the device with which it is interfering

Warnings

- The use of accessories, transducers and cables other than those specified, with the exception of transducers and cables sold by the manufacturer of the Doppler as replacement parts for internal components, may result in increased emissions or decreased immunity of the Doppler.
- The Doppler should not be used adjacent to or stacked with other equipment and that if adjacent or stacked use is necessary, the Doppler should be observed to verify normal operation in the configuration in which it will be used.
- Portable RF communications equipment (including peripherals such as antenna cables and external antennas) should be used no closer than 30 cm (12 inches) to any part of the Doppler including cables specified by the manufacturer. Otherwise, degradation of the performance of this equipment could result.